

PUMP DISCHARGE or PRESSURIZED LINE

1" ON/OFF FULL BORE BALL VALVE

3-5 GPM @ 15 PSIG (MIN)


~10"

CT103/25 SENSOR SUPPLIED BY CERLIC

13"

2"


2"

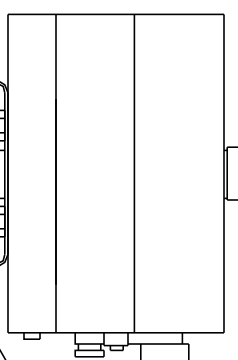


1" 3-WAY BALL VALVE, T-PORT
REQ'D 60 PSIG AIR, 1/4" NPT FITTING
FLUSH WATER TO BACKWASH SENSOR
(REQ'D +15 PSIG OVER FLUID PRESSURE)

1" THROTTLING BALL VALVE
1" SAMPLING VALVE


TO PUMP SUCTION or SUPPLY TANK

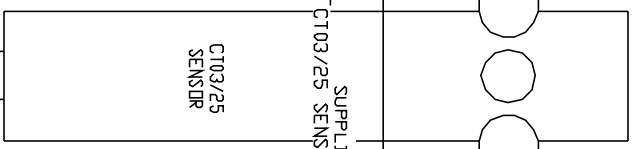

10-3/4"

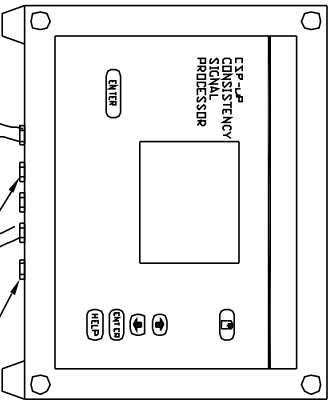

13"

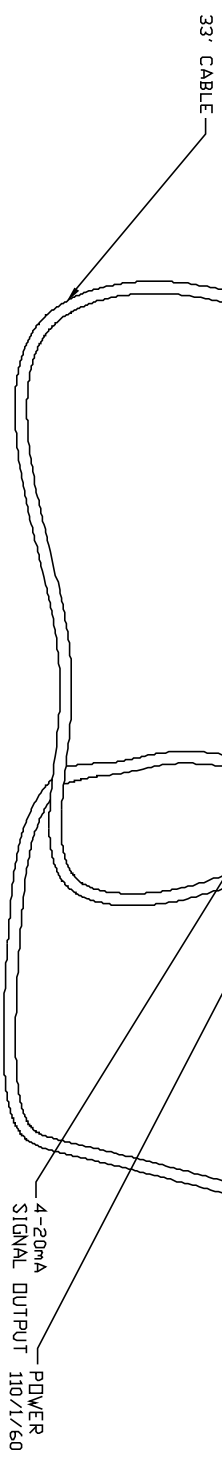

33' CABLE

4-20mA SIGNAL OUTPUT
POWER 110/1/60



Cerlic Environmental Controls, Inc

P.O. Box 420097

Atlanta, GA 30342

Phone (404) 256-3097

Fax (404) 256-3094

CERLIC HIGH SOLIDS METER

CT03/25 W/ 3-WAY

FLUSH VALVE

DRAWING NUMBER

107A

PROJECT NUMBER

CT03/25

SCALE

1/4

DATE	BY	CHKD BY	APP'D BY
1	TJJ		
2	SKM		
3	JR		
4			
5			
6			
7			